


Summary of Regulatory Licenses for Node Seeker 2000

- 1- US FDA - Class 1- Exempt from 510(k)- GMP license number **74527**



- 2- EU CE marking: **CE665492**

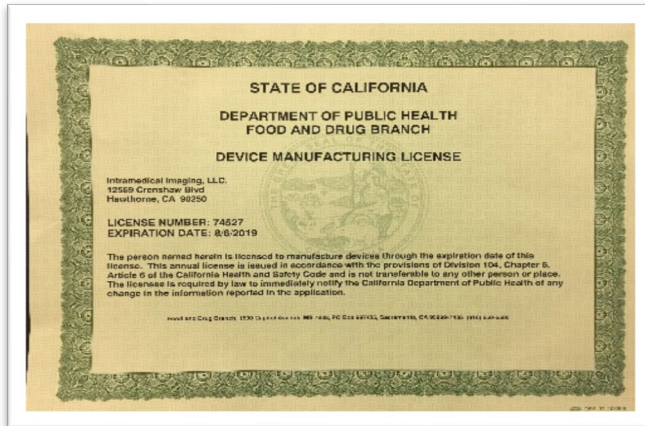

Donawa Life Sciences Srl
Piazza Albania, 10
00153 Roma, Italy



3- ISO 13485 – certificate number **FM 659427**



4- Sterilization validation- **Report #RPT04081 by ASP**

Sterilization validation of the Wireless Gamma Probe (P/N: WG-140A), provided by Intramedical Imaging, was performed in the STERRAD® 100NX Sterilization System following the "overkill sterilization method" referenced in AAMI Standards and Recommended Practices: ISO 14937 (2009)



ADVANCED STERILIZATION PRODUCTS

Division of Ethicon, Inc.
a Johnson & Johnson company

STERILIZATION VALIDATION REPORT

SPONSOR: INTRAMEDICAL IMAGING
TEST ARTICLE: WIRELESS GAMMA PROBE (P/N: WG-140A)
TITLE: STERILIZATION VALIDATION OF WIRELESS GAMMA PROBE FROM INTRAMEDICAL IMAGING IN THE STERRAD® 100NX STANDARD CYCLE
NUMBER: RPT04081

Test Report Number: T150914D06-E

Issued to:

Cybernet Manufacturing
5 Holland Irvine, California 92618

Issued by:

Compliance Certification Services Inc.
Xindian Lab.
No.163-1, Jhongsheng Rd., Xindian Dist.,
New Taipei City, 23151 Taiwan.
TEL: 886-2-22170894
FAX: 886-2-22171029
Issued Date: September 17, 2015



Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document. The client should not use it to claim product endorsement by TAF, A2LA, NIST or any government agencies. The test results in the report only apply to the tested sample.

5- EMC 60601-1-2 & Electrical safety 60601-1 of the control unit (T10C)

CCSRF Compliance Certification Services Inc.

Report No.: T150914D06-E

CE EMC TEST REPORT

for

Medical / enterprise Tablet

MODEL: T10C; CyberMed T10C; Cybernet T10C

Test Report Number: T150914D06-E

Issued to:

Cybernet Manufacturing
5 Holland Irvine, California 92618

Issued by:

Compliance Certification Services Inc.
Xindian Lab.
No.163-1, Jhongsheng Rd., Xindian Dist.,
New Taipei City, 23151 Taiwan.
TEL: 886-2-22170894
FAX: 886-2-22171029
Issued Date: September 17, 2015



Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document. The client should not use it to claim product endorsement by TAF, A2LA, NVLAP, NIST or any government agencies. The test results in the report only apply to the tested sample.



6- EMC 60601-1-2 & Electrical safety 60601-1 of the NS2000

COMPATIBLE ELECTRONICS IEC / EN 60601-1-2 Report Number: D70621Q1 Page 1 of 32

**IEC / EN 60601-1-2
3RD EDITION
TEST REPORT**

for
NODE SEEKER
MODEL: NS-2000

PREPARED FOR
INTRAMEDICAL IMAGING, LLC
12569 CRENSHAW BLVD.
HAWTHORNE, CA 90250

Prepared by: *Joey Madlangbayan*
JOEY MADLANGBAYAN

Reviewed by: *Matt Harrison*
MATT HARRISON

COMPATIBLE ELECTRONICS INC.
20621 PASCAL WAY
LAKE FOREST, CALIFORNIA 92630
(949) 587-0400

DATE: SEPTEMBER 15, 2017

REPORT BODY	APPENDICES					TOTAL
	A	B	C	D	E	
PAGES	2	1	2	2	2	9
						82

This report shall not be reproduced, except in full, without the written approval of Compatible Electronics.

NVLAP TESTING
NVLAP LAB CODE 200527-0

IAC-MRA

COMPATIBLE ELECTRONICS Page 1 of 55
Report Number: D70712S1
Standard: IEC 60601-1

**CONFORMANCE
TEST REPORT
FOR
Model: NS2000**

Prepared for
Intra Medical Imaging, LLC 12569 Crenshaw Blvd Hawthorne, CA 90250

Prepared By: *Joey Madlangbayan*
Joey Madlangbayan
Product Safety Manager

Reviewed By: *Matt Harrison*
Matt Harrison
Lab Manager


NVLAP TESTING
NVLAP LAB CODE 200527-0

IAC-MRA



Intra Medical Imaging LLC

7- TaiwanFDA

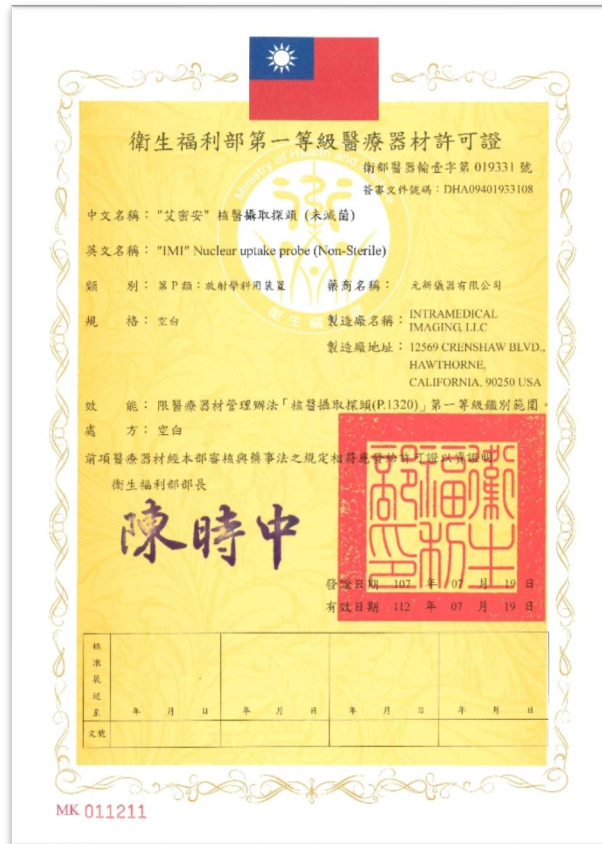

12569 Crenshaw Blvd. Hawthorne, CA 90250
Phone: (424) 456-7316
Fax: (424) 456-7195